

GPIO Deployment Guide

SENSARRAY+

SENSARRAY PRO AND ENTERPRISE

SENSX EXTREME



Legal Notices

Copyright ©2017-2021 SensThys Inc. All rights reserved.

SensThys has intellectual property rights relating to technology embodied in the products described in this document, including without limitation certain patents or patent pending applications in the U.S. or other countries. This document and the products to which it pertains are distributed under licenses restricting their use, copying, distribution and de-compilation. No part of this product documentation may be reproduced in any form or by any means without the prior written consent of SensThys Corporation and its licensors, if any. Third party software is copyrighted and licensed from Licensors. SensThys, SensArray and other graphics, logos, and service names used in this document are trademarks of SensThys in the U.S. and other countries. All other trademarks are the property of their respective owners. U.S. Government approval required when exporting the product described in this documentation.

Federal Acquisitions: Commercial Software -- Government Users Subject to Standard License Terms and Conditions. U.S. Government: If this Software is being acquired by or on behalf of the U.S. Government or by a U.S. Government prime contractor or subcontractor (at any tier), then the Government's rights in the Software and accompanying documentation shall be only as set forth in this license; this is in accordance with 48 C.F.R. 227.7201 through 227.7202-4 (for Department of Defense (DoD) acquisitions) and with 48 C.F.R. 2.101 and 12.212 (for non-DoD acquisitions).

DOCUMENTATION IS PROVIDED "AS IS" AND ALL EXPRESS OR IMPLIED CONDITIONS, REPRESENTATIONS AND WARRANTIES, INCLUDING ANY IMPLIED WARRANTY OF MERCHANTABILITY, FITNESS FOR A PARTICULAR PURPOSE OR NON-INFRINGEMENT ARE HEREBY DISCLAIMED, EXCEPT TO THE EXTENT THAT SUCH DISCLAIMERS ARE HELD TO BE LEGALLY INVALID.

FCC Compliance

This equipment has been tested and found to comply with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

Any change or modification to this product voids the user's authority to operate per FCC Part 15 Subpart A. Section 15.21 regulations.

Industry Canada Compliance

This device complies with Industry Canada License-exempt RSS standards. Operation is subject to the following two conditions: (1) this device may not cause interference and (2) this device must accept any interference, including interference that may cause undesired operation of the device. This device has been designed to operate with a variety of different gain (dBi). The reader maximum output power is set by the gain of the antenna. Using an antenna having a higher gain is strictly prohibited per regulations of Industry Canada. In addition, using the reader at a power exceeding the maximum output power for a given antenna is also strictly prohibited. The required antenna impedance is 50 ohms. To reduce potential radio interference to other users, the antenna type and its gain should be so chosen that the equivalent isotropically radiated power (EIRP) is not more than that required for successful communication.

Conformité d'Industrie Canada

Cet appareil est conforme aux normes RSS exemptées de licence d'Industrie Canada. L'opération est soumise aux deux conditions suivantes: (1) cet appareil ne doit pas provoquer d'interférence et (2) cet appareil doit accepter toute interférence, y compris les interférences susceptibles de provoquer un fonctionnement indésirable de l'appareil. Cet appareil a été conçu pour fonctionner avec une variété de gains différents (dBi). La puissance de sortie maximale du lecteur est définie par le gain de l'antenne. L'utilisation d'une antenne ayant un gain plus élevé est strictement interdite par règlement d'Industrie Canada. En outre, l'utilisation du lecteur à une puissance supérieure à la puissance de sortie maximale pour une antenne donnée est également strictement interdite. L'impédance d'antenne requise est de 50 ohms. Afin de réduire les interférences radio potentielles avec d'autres utilisateurs, le type d'antenne et son gain devraient être choisis de manière à ce que la puissance émise isotropiquement (EIRP) équivalente soit supérieure à celle requise pour une communication réussie.

Caution

Reader antennas should be positioned so that personnel in the area for prolonged periods may safely remain at least 31 cm (12.2 in) in an uncontrolled environment from the antenna's surface. See FCC OET Bulletin 56 "Hazards of radio frequency and electromagnetic fields" and Bulletin 65 "Human exposure to radio frequency electromagnetic fields."

Vorsicht

Reader Antennen sollten so positioniert werden, dass das Personal im Bereich über einen längeren Zeitraum kann sicher bleiben mindestens 31 cm (12.2 Zoll) entfernt von der Antenne Oberfläche, in einer unkontrollierten Umgebung. Siehe FCC OET Bulletin 56 "Gefahren der Radiofrequenz und elektromagnetische Felder" und Bulletin 65 "Human Exposition gegenüber hochfrequenten elektromagnetischen Feldern."

Revision History

Version	Author	Date	Changes
1.0		2017	Initial Document
1.1		2018	
1.2		2018	
1.3	Robert Ma	2019-05-01	Add SensArray Gen2 and Extreme GPIO definitions
1.4	Jo Major	2020-2-14	Add clarification and examples. Anode/Cathode discussion with figures.
V2.0- V2.1			Minor updates
V2.2	N. Mitchell	2021-11-12	Updated Copyright

Table of Contents

LEGAL NOTICES	2
REVISION HISTORY	3
TABLE OF CONTENTS.....	4
CHAPTER 1 INTRODUCTION	6
Safety Advisory	6
CHAPTER 2 GPIO ON SENSARRAY READERS	7
Interface Specifications.....	7
GPIO General Description	7
Power Sourcing.....	7
Input Signals - State of External Devices	8
Output Signals - Control of External Devices	8
SensArray+ GPIO Pin-out.....	9
Wiring the GPIO	9
CHAPTER 3 EXAMPLES AND CONSOLE INTERFACE	10
Examples Using Input and Output Pins and 24 v.....	10
Example 1: Using Internal 24VDC to power external device.....	10
Example 2: Using External 24VDC to power external device.....	12
Example 3: Connecting PIR (Passive Infrared) to Internal Input	13
Configuring and Testing with the RFID Console	14
Powering the 24VDC System	14
Testing your GPIO Input	14
Testing GPIO Output.....	15
Programming the GPIOs	15

Important Note	15
API Interfaces	15
GPI Notifications.....	16
CHAPTER 4 GPIO ON ENTERPRISE	17
GPIO Pin-out Specifications.....	18
CHAPTER 5 GPIO ON SENSX EXTREME	19
Digital Interface Specifications.....	19
GPIO (General Purpose Input/Output) Connector	19
GPIO and GPIO Cable Pin-out Specification	20
CHAPTER 6 TROUBLESHOOTING.....	20
Common Anode → SensArray+, Pro and Enterprise	22
Common Cathode → Extreme	23
Reversible Common Cathode or Anode → All	24

CHAPTER 1 Introduction

This Hardware Setup Guide provides instructions for installing and operating the GPIO connection on the following units:

- SensArray+
- SensArray Pro
- SensArray Enterprise
- SensX Extreme

This document is designed for use by RFID system integrators, IT networking professionals, and software developers - those who wish to develop RFID, networking solutions, and agile power deliver systems to take full advantage of the unique capabilities of the SensArray.

At SensThys.com, the user can find substantial additional information about RFID.

- **User Guide** – an overview of the interfaces for the SensArray, including General Purpose Input/Output (GPIO), POE, SMA outputs for antennas, DC power input, POE inputs.
- **Upgrade Guide** – instructions for the user to upgrade the firmware of the SensArray while in field operation. The SensArray can be upgraded through any Ethernet port on the unit.
- **Developer's Guides** – Programming Interfaces and Example Code.

Safety Advisory

This guide discusses wiring electrical devices to the SensArray+ GPIO ports. The voltage levels that are supplied from the SensArray+ are limited to 24VDC. Although this voltage level is generally not a hazard, under some conditions it could provide a significant shock. Also, wiring devices live could generate unusual current paths between the SensArray+ and your external equipment before ground and voltage connections are set up properly, possibly resulting in harm to the SensArray+ or your equipment.

SAFETY WARNING

Power down the SensArray+ device and all equipment you are connecting to the GPIO port before doing the wiring!

Chapter 2 GPIO on SensArray Readers

Interface Specifications

Feature	Specification
GPIO (incl. Input power, output power)	4 input, 4 output; 24VDC supplied by reader Pin 11 GND Pin 12 Connection for external 24VDC Pin 1 GND Pin 2

GPIO General Description

This integrated reader contains a 24V power supply! Gone is the need for extra power supplies and the dreaded GPIO box.

The SA+ and Pro provide up to 15W of power, the Enterprise provides up to 30W of power to drive those GPIO devices.

The SensArray+ GPIO port provides four control inputs and four outputs. The SensArray+ and Pro GPIO is not optically isolated, while the Enterprise features optical isolation on all ports. When operational both the input and output pins are fully interfaced to the electrical systems.

The GPIO operation contains three general aspects. These include power sourcing, accepting digital signals through one of the inputs, and turning external devices on and off through the outputs.

Power Sourcing

To use the GPIO, the reader should be connected to external ground via pins 2 and/or 12. These pins are internally connected within the reader.

External devices can be powered in two different ways.

1. External devices can be powered from the reader. This power can be delivered to the external device via pin 11, which provides a switched 24 VDC to a maximum of 600 mA. Users should bear in mind that using power from the reader decreases the amount of power that can be provided to other POE or GPIO devices. See Figure 2 below.

2. External devices can be powered by an external power supply, with the reader controlling the devices. To use an external power source connect the +24VDC to Pin 1 and ground to Pin 2 or Pin 12. See Figure 3 below.

In this situation the power consumed by the external devices does not reduce the power that the reader can provide. Note, external power sources do not provide power to POE devices.

Pin 1 provides TVS surge protection and can help prevent surges in the 24 VDC supply from being passed onto external devices.

Input Signals - State of External Devices

Users may provide input signals to the reader via the GPIO inputs.

- A signal is considered a “1” if the voltage at the input pin is between 5V and the 24V upper rail.
- A signal will be treated as a “0” if the voltage at the input pin is between 0 and 3.3V. Signals between 3.3V and 5V are not recommended. These analog “on” voltage ranges are detected by circuitry within the reader, and then presented as true digital signals to the microprocessor.

The input connections at Pins 7 through Pin 10 are addressed as Input 1 through Input 4, respectively. See Table 1 below.

There is no linkage between the inputs and outputs. Each input or output operates independently from other inputs and output.

Output Signals - Control of External Devices

The function of the four output pins is to provide a switch to ground. The concept of switching on the ground side may be counter-intuitive, please carefully look at the various wiring diagrams.

- When the output is “off”, the switch is open, and no current can flow into the output pin.
- When the output is “on”, the switch is closed and current may flow directly into the output pin.

The output connections at Pins 3 through Pin 6 are addressed as Output 1 through Output 4, respectively. See Table 1 below.

SensArray+ GPIO Pin-out

PIN Number	Description
Pin 1	Up to 24VDC External
Pin 2	Ground
Pin 3	External Output 1
Pin 4	External Output 2
Pin 5	External Output 3
Pin 6	External Output 4
Pin 7	External Input 1 (High is 5-24VDC)
Pin 8	External Input 2 (High is 5-24VDC)
Pin 9	External Input 3 (High is 5-24VDC)
Pin 10	External Input 4 (High is 5-24VDC)
Pin 11	+24VDC Internal
Pin 12	Ground

Table 1: GPIO Pinout for SensArray+

Wiring the GPIO



Figure 1 The GPIO port.

Wires, recommended solid 20-26 AWG, are inserted into the round openings. To remove the wires, a small tool is inserted into the rectangular slot above, allowing the wired to be easily pulled out. Pin 1 is marked at the far left.

As detailed in Table 1 above, Pin 11, the second from the right of the picture above, can be used to source 24VDC. Either Pin 2 or Pin 12 can be used as the ground.

Note that in determining whether you can use the 24VDC, you also must look at the overall power consumed by other devices in the reader network as well as the power consumed by the RF radio when reading tags. If this greater than the available power, you can use an

external power supply to drive your external devices. You just need to connect the positive side of your DC voltage supply to Pin 1 and the ground side to Pin 2.

Chapter 3 Examples and Console Interface

Examples Using Input and Output Pins and 24 v

Example 1: Using Internal 24VDC to power external device

In this example, the output pin 5 is used to turn on or off a load, such as a light or a motion sensor. The 24VDC is used to power the load, so that an external power supply is not needed.

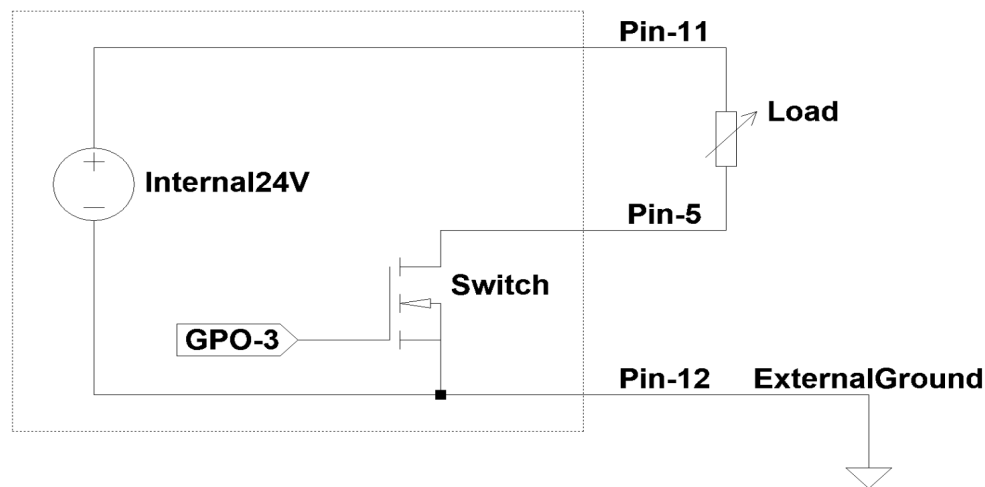


Figure 2: Using the GPIO to control an external device powered by 24VDC Internal supply

Figure 2 illustrates a load that is powered by the Internal 24VDC supply connected via Pin 11 of the GPIO connector. Pin 5 is used to control turning on or off the load. In this case, the circuit is set up to flow current through the load into Pin 5 External Output “3”.

- When the switch is closed by the control signal GPO-3, current flows activating the load.
- When the switch is open, no current flows and the load will be inactive.

Note that Pin 12 is connected to an external ground in this figure.

However, if Pin 5 was connected to a control signal, that signal could open a path inside the load that would need the current return path back through Pin 12. In this case where Pin 5 is connected to a control signal, a pull-up or pull-down resistors will be needed to ensure that the control voltages are appropriate for activating and deactivating your device.

Example 2: Using External 24VDC to power external device

In this example, the load is powered by an external 24VDC power supply. Pin 5 output is used to control turning on or off the load such as a light or a motion sensor. 24VDC is supplied to Pin1 of the SensArray and the load. Pin 2 ground is used in this case.

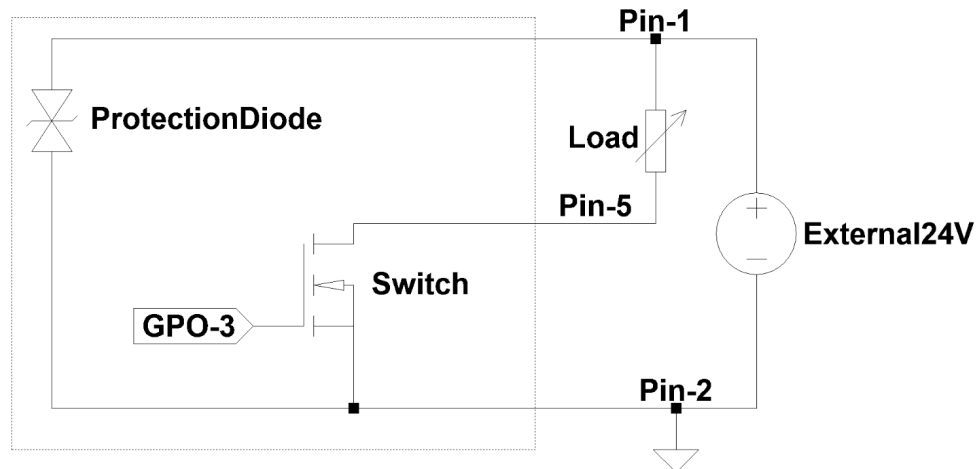


Figure 3 Using the GPIO to control an external device powered by an external supply

Figure 3 depicts the an external 24VDC supply connected to Pin 1 and external ground to Pin 2. An external load is supplied power by the external 24VDC source which has been also connected to Pin 1.

- The current path to ground for the accessory is in through Pin 5, through the switch controlled by GPO3, and back out to the accessory ground through Pin 2.
- When the microprocessor turns GPO3 “on”, it activates the switching FET, which effectively takes Pin 5 to ground, turning on the load device.
- When the microprocessor turns GPO3 “off”, no current flows and the load is inactive or off.

Note that in this case, the external 24VDC connected through Pin 1 is bridged to ground through a transient voltage suppression device to help reduce electronic noise in the circuit.

Example 3: Connecting PIR (Passive Infrared) to Internal Input

Passive Infrared switch will detect infrared body signature, switch an output signal to indicate detection, and hold the “active” state until detection is cleared.

In this example, the PIR switch is powered by the reader via Pin 11 (Pin 12 gnd), and the status output is fed to the GPIO connector Pin 7 Input #1. This signal is then used by the reader to enable reading tags, as would be attached to the infrared emitter (body) that triggered the PIR switch in the first place.

When the PIR is inactive, Pin 7 will be “High”, or > 5 VDC, pulled up to V+ thru the 4k ohm resistor.

When the PIR is active, Pin 7 will be “Low”, or < 2.2 VDC, where V- from the PIR is shorted to gnd.

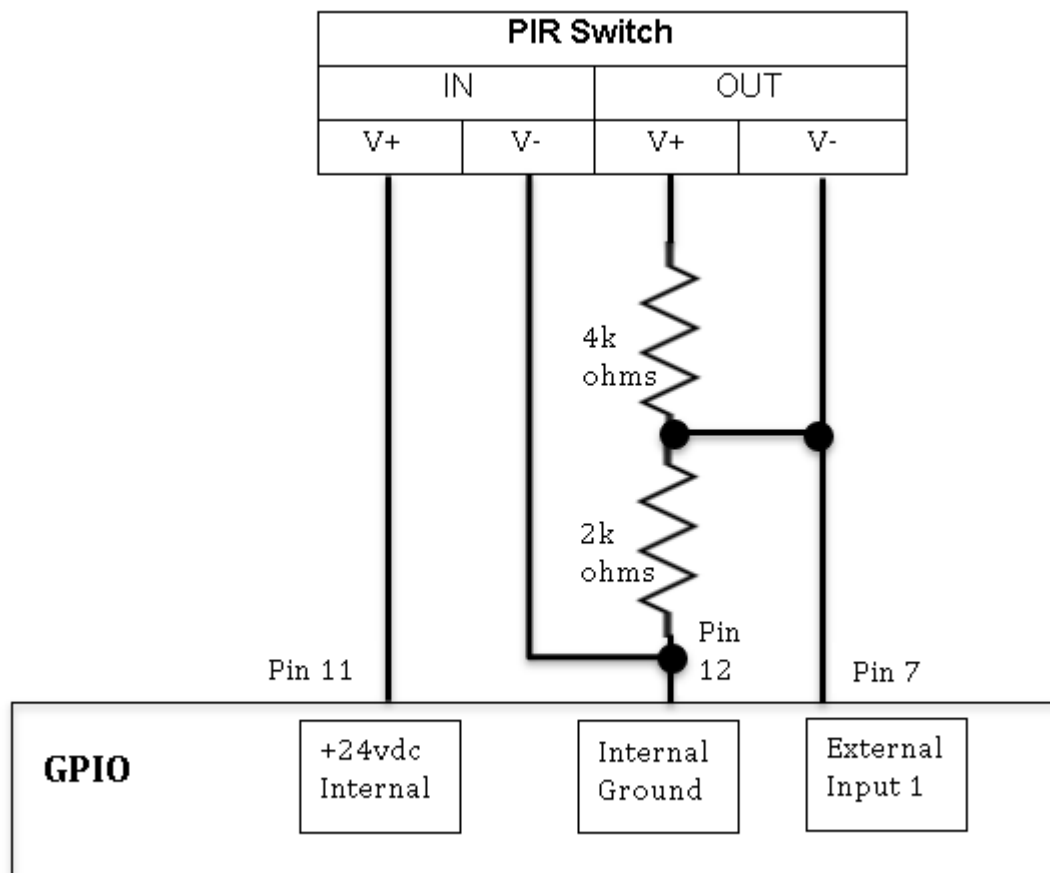


Figure 4 Wiring schematic with a PIR

Configuring and Testing with the RFID Console

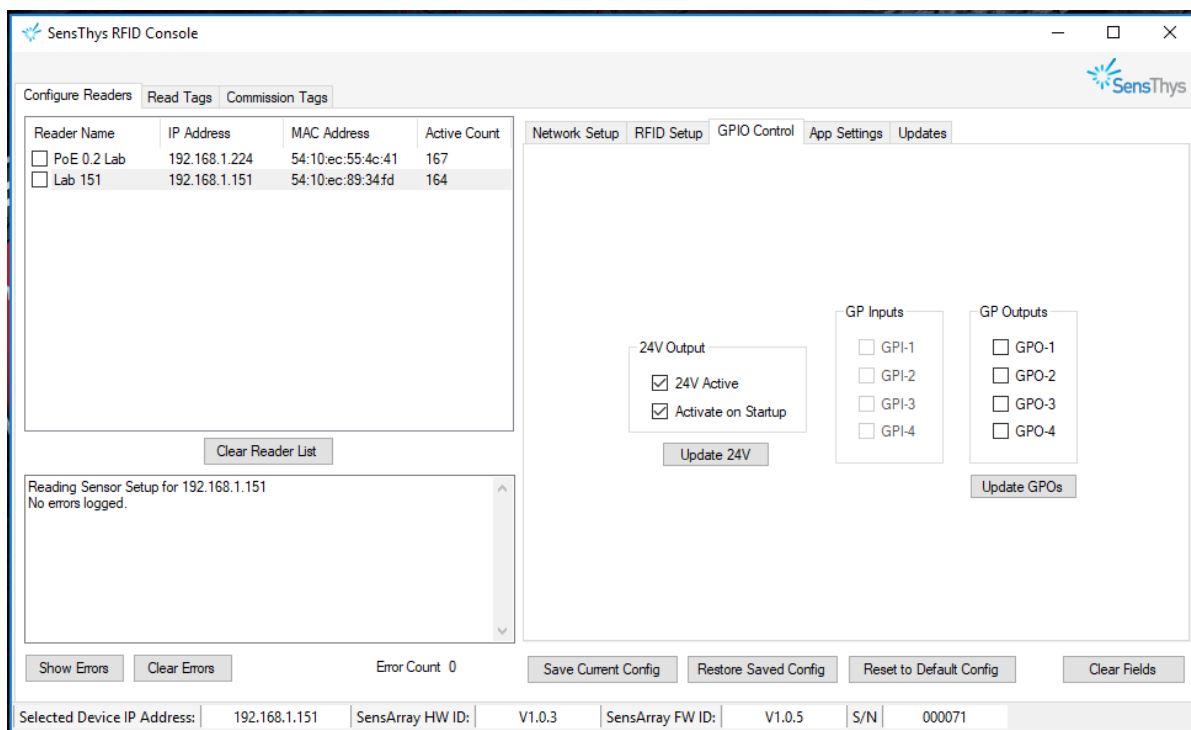


Figure 5 GPIO Control tab.

Powering the 24VDC System

The SensArray+ can source 24VDC power through Pin 11. If you are going to use the SensArray+ to power GPIO accessories, you should start with the SensArray+ powered, but with nothing connected to the GPIO. Check the “24V Active” and “Activate on Startup” boxes, hit the “Update 24V”, and finally click “Save Current Config” on the GPIO tab.

Disconnect the power from your SensArray+, then connect your external ground to Pin 2. At this point the SensArray+ should be restarted.

Testing your GPIO Input

It is quite simple to test your General-Purpose Inputs. To do so, simply click on the “Update GPOs” button below the “GP Outputs” section. The current state of each of the inputs will be read and displayed as unchecked if the voltage is low (below 3.3VDC) on the associated input line or checked if it is above 5VDC. Note that values between 3.3VDC and 5VDC will read but should be considered indeterminate relative to reliable operation of your system.

Once you have verified the current state of your GPIs, you should change the state of each input – preferably one at a time – and verify that each one correctly changes the associated checked item in the “GP Inputs” section. Note that a notification message is sent from the SensArray+ to the RFID Console application whenever general-purpose inputs change. The RFID Console receives the message and changes the check box that indicates the new state of the input (or inputs) that changed.

Testing GPIO Output

Testing your General-Purpose Outputs proceeds along similar lines. Set up your hardware configuration, then check, or uncheck each associated check box in the GP Outputs group in the interface. After changing the check box, click the “Update GPOs” button to change the state of the output line. Observe whether your external device responds correctly when you activate or deactivate the output.

If you have difficulty when testing either the GPIs or the GPOs, be sure to check both the power supply connections as well as the connections to your external input or output devices. If those all appear correct and you still have problems, the next step is to use a multimeter and check voltage values for the inputs or outputs. As described above, the inputs must be below 3.3VDC to be off and above 5VDC (and below 24VDC) to be considered on. For GPOs, when the GPO is activated, the output line should be pulled to ground and when deactivated should pull up to your high voltage level.

Programming the GPIOs

There are three interfaces for programming the GPIOs available in the RFID.dll API. You can find detailed documentation of the interfaces in the “GPIO and 24V Management Methods” section of Appendix B in “The SensArray Programming Guide”. A brief overview of using these functions is provided here.

Note that the inputs are debounced in software, so you do not need to provide your own debouncing routine.

Important Note

When the reader is reading tags while in a continuous inventory cycle, the only command that can be sent to the SensArray reader is the stop command. As a consequence, you cannot call the API method, `GetGPIOSetup()` discussed below, to determine the state of the general-purpose inputs. A UDP notification mechanism has been provided to inform your application when an input changes from on to off or vice versa. This notification is discussed in the section, “*GPI Notifications*” below.

API Interfaces

As described above, you can configure the 24VDC setup through the RFID Console application. However, if you want to provide similar functionality through your application, you would use the `Get24VStatus()` and `Set24VStatus()` methods to do so. Also, if you want to have more control over when you activate the internal 24VDC supply from your application, you would use `Set24VStatus()` to do so.

If you want to query the current state of all of your GPIs and GPOs, you would use the `GetGPIOSetup()` method to do so. A call to this method returns a Byte whose bits provide the state of each of the 4 inputs and 4 outputs as follows [$i_4, i_3, i_2, i_1, o_4, o_3, o_2, o_1$] where i_n will be 1 if the input is high and 0 if it is low and o_n will be 0 if the output is not activated and 1 if it has been activated. As an example, if output 1 is high, output 2, 3 and 4 are low,

input 3 is high, and inputs 1, 2, and 4 are low, the call to `GetGPIOSetup()` will return 0x41. Also, for completeness, output 1 is wired into pin 3, and input 3 is wired into pin 9.

To set the state of the GPOs, you use the method `SetGeneralPurposeOutputs()`. This method uses a set of bits similar to the value returned for `GetGPIOSetup()` described above. You send a Byte value as follows `[0, 0, 0, 0, o4, o3, o2, o1]` where o_n is set to 0 to deactivate the associated output and 1 if it is to be activated. Note that this is not a masked operation, so to change the state of an output, you should read the current state, change the value of the bits corresponding to the output(s) you want changed, then write the new data.

GPI Notifications

To eliminate the need to poll the state of the General-Purpose Inputs from your application and to provide a way for your application to know when a GPI changes state, a notification message is broadcast to the local subnet on UDP port 3984. This notification is sent as soon as a change on any of the GPI input pins is detected. Once you receive this type of notification, your application can take the desired action which might include activating GPOs, starting tag read cycles, etc. Similarly, by listening for these messages during tag inventory cycles, your application can detect a change in an input that could trigger your application to send the command to stop the tag inventory process.

The format of the notification messages is as follows:

Bytes 1,2,4,9,14: Reserved for future use

Byte 3: Total message length in bytes = data length + 19. This should be 20 for a GPI change notification.

Bytes 5-8: The four bytes of the IP address of the reader sending the notice.
IP Address = `msg[4].msg[5].msg[6].msg[7]`

Bytes 10-13: These 4 bytes provide a 32-bit value for the reader uptime in seconds from when the unit booted until the time this notification was sent.

Bytes 15-18: These 4 bytes can be reconstituted into a 32-bit value providing a sequence number for the notification. Since there can potentially be multiple paths from the reader to your application, this sequence number can be used to filter out duplicates.

Byte 19: The notification type. For GPI notifications, this value is 16 (hex 0x10)

Byte 20: This byte provides the new GPI state as follows `[0, 0, 0, 0, i4, i3, i2, i1]` where i_n is set to 0 when the input is low and 1 when the input is high.

Chapter 4 GPIO on Enterprise

These three readers have the same generation RF module and computer controller. However, the PRO model's GPIO functionality is identical the SensArray+. Refer to Chapter 2 for information on the SensArray Pro's GPIO functionality.

The GPIO information in this chapter is specifically for the SensArray models listed below:

- Enterprise

The main differences in GPIO functionality between these models and the original SensArray+ reader are:

- Enterprise Input and Output pins are opto-isolated.
- On the Enterprise, Pin 1 and 11 are 24VDC **output voltage** connections only. The SensArray can provide 24vdc to power external devices, sourcing up to 1.2 A when pins 1 and 11 are tied together.

See Chapter 3 for examples of how to use the Output pins and 24VDC power supply, as well as programing the input and output GPIO lines.

GPIO Pin-out Specifications

The pinout assignments for the GPIO below:

Pin Number	Enterprise	SA+ and Pro
Pin 1	+24VDC output, max sourcing current 1.2 A	+24 VDC external (same as SensArray+)
Pin 2	External ground, for Pin 1 use	
Pin 3	Output 1	
Pin 4	Output 2	
Pin 5	Output 3	
Pin 6	Output 4	
Pin 7	Input 1 ($V < 1$ VDC = "0", $5 < V < 24$ VDC = "1")	
Pin 8	Input 2 ($V < 1$ VDC = "0", $5 < V < 24$ VDC = "1")	
Pin 9	Input 3 ($V < 1$ VDC = "0", $5 < V < 24$ VDC = "1")	
Pin 10	Input 4 ($V < 1$ VDC = "0", $5 < V < 24$ VDC = "1")	
Pin 11	+24VDC output, max sourcing current: <ul style="list-style-type: none"> 1.2 A for Enterprise 600 mA for Pro 	
Pin 12	External ground, for Pin 11 use	

Table 2: GPIO Pins for SensArray One Pro, Pro and Enterprise



Figure 6 The GPIO port, labeled "I/O"

Wires, recommended solid 20-26 AWG, are inserted into the round openings. To remove the wires, a small tool is inserted into the rectangular slot above, allowing the wires to be easily pulled out. Pin 1 is marked at the far left.

Chapter 5 GPIO on SensX Extreme

This section is specifically for the SensX Extreme reader.

The main differences in GPIO functionalities between the Extreme reader and the other SensArray readers are:

- Extreme reader has 2 input and 2 output pins, instead of 4 input and 4 output pins.
- The +24 vdc pin is a Vcc **input voltage connection**, that is used as the rail for output “HI” on the GPIO output pins 2 and 4.

See Chapter 3 for examples of how to use the Output pins and 24VDC power supply, as well as programing the input and output GPIO lines.

Digital Interface Specifications

Feature	Specification
GPIO (incl. Input power)	2 input, 2 output, optically isolated; +12 to 24VDC input and gnd; Rugged IP67 6-pin circular male pin connector with dust cap

GPIO (General Purpose Input/Output) Connector

The SensX Extreme GPIO port provides two inputs and two outputs, which are all opto-isolated. The connector also has an input pin for +24 VDC to power the GPIO outputs as well as power the Extreme unit.

The pinout assignments for the two control inputs and two control outputs are below.

For the GPIO output pins 2 and 4 to switch, Vcc (+12-24 VDC) be connected to Pin 1 and external ground to pin 6. Output Hi or “1” will then be tied to the rail voltage on Pin 1.

Toggling the external outputs opens or closes an internal transistor switch that allows/prevents current to flow from the voltage applied to the external output pin to ground.

The Extreme unit can be powered by connecting +12 to +24 VDC to pin 1, and ground to pin 6.

GPIO and GPIO Cable Pin-out Specification

The pin-out of the GPIO is given below.

SensThys provides an optional connector cable which is fully IP67 when used with the Extreme. The wiring of the cable is as follows:

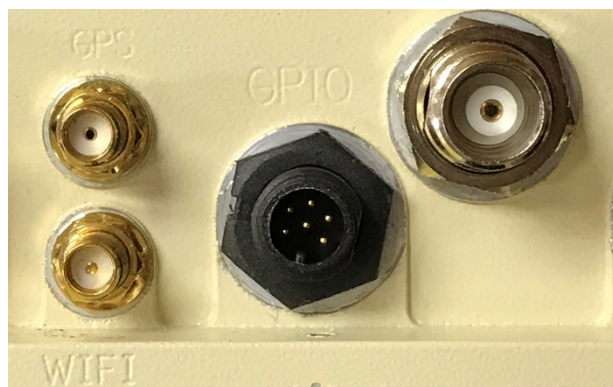


Figure 7 GPIO connector on Extreme

Pin	Assignment	Wire Color	Description
1	Input 2	White	V<1, Low. 5-24V, High
2	Ext Ground	Black	Connect to external ground
3	Input 1	Blue	V<1, Low. 5-24V, High
4	Output 2	Yellow	When Output = "1", V (pin 4) = voltage at Pin 5 (VCC)
5	VCC	Red	Input Voltage (5-24V)
6	Output 1	Green	When Output = "1", V (pin 4) = voltage at Pin 5 (VCC)

Table 3: GPIO Pins for Extreme

Chapter 6 Troubleshooting

Why doesn't my light work? Buzzer is quiet?

The world of light stacks and GPIO devices is intriguing. At the lower end on the cost side, there are \$15 devices that you can purchase completely without any documentation. At the high side are \$200 IP67 devices with absolutely clear wiring schematics. At least spend enough money to get a clear schematic, it will save you lots of time.

There are three basic wiring configurations, this is the basic purchasing information you need.

Common Anode → SensArray+, Pro and Enterprise

All of the “high” sides of the various devices are connected to 24VDC.

The switching occurs on the ground side.

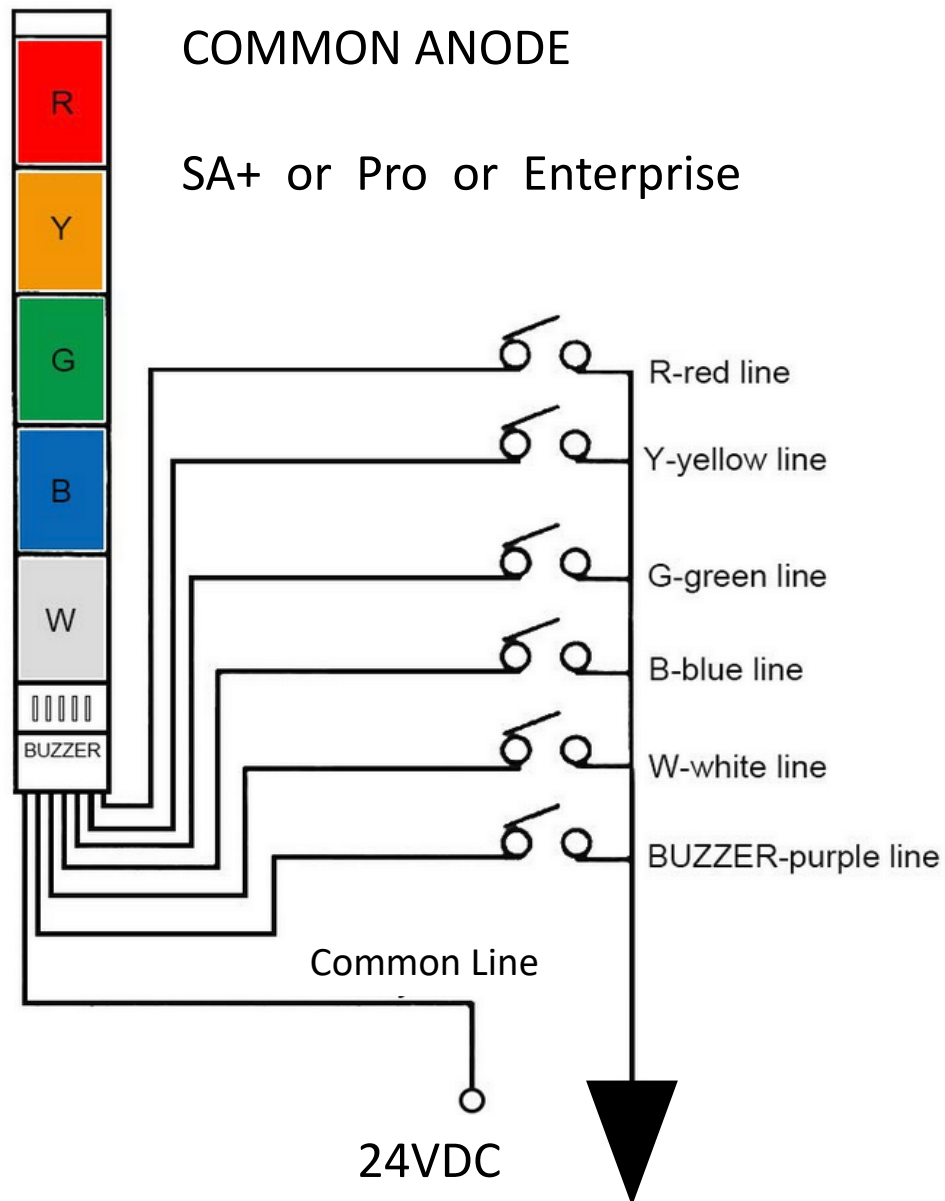


Figure 8 A COMMON ANODE configuration. This works for Enterprise, Pro or SA+.

A common anode device will NOT work with Extreme.

Common Cathode → Extreme

All of the “low” sides of the various devices are connected to GROUND.

The switching occurs on the +24 VDC side.

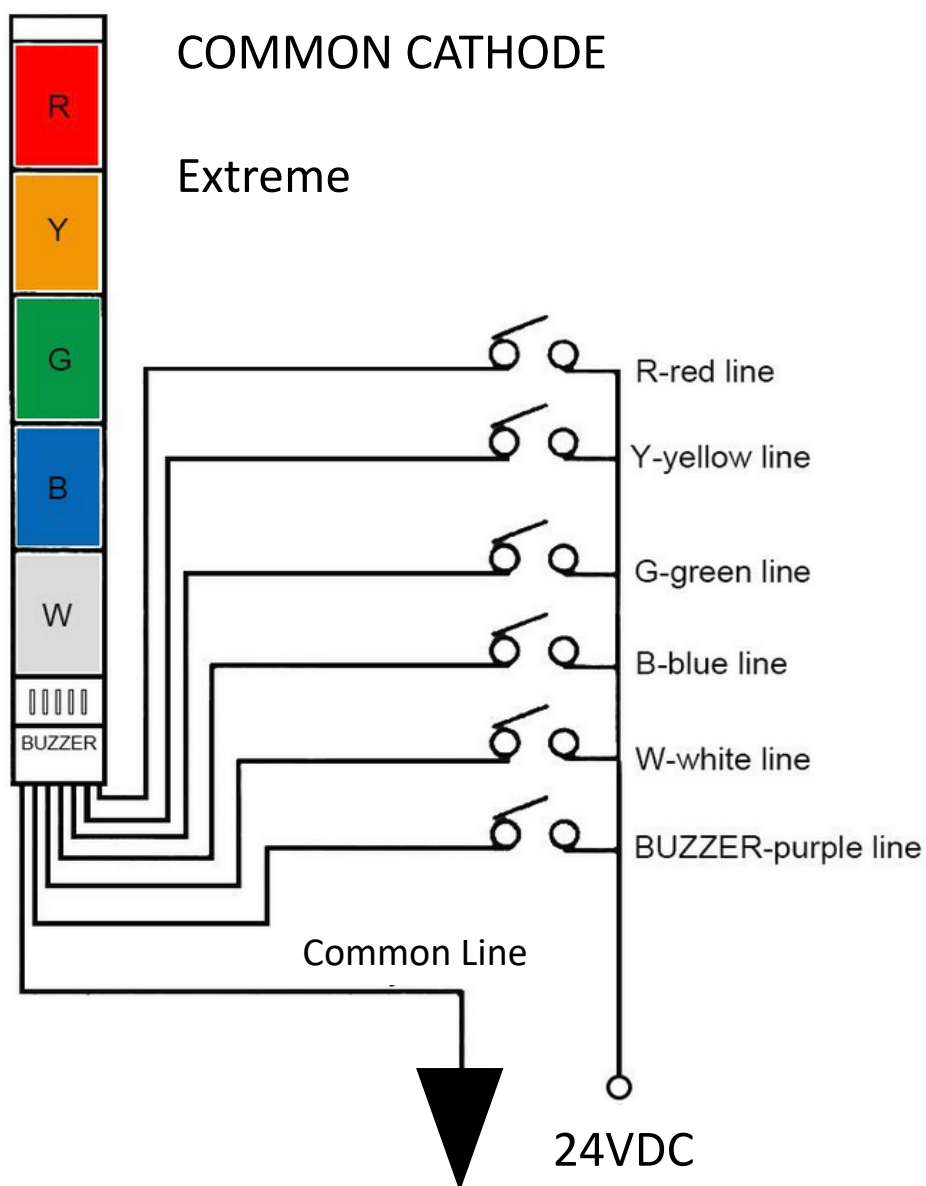


Figure 9 A COMMON CATHODE configuration. This works with Extreme.

A common cathode device will NOT work with SensArray+, Pro or Enterprise.

Reversible Common Cathode or Anode → All

Either the “low” or “high” sides of the various devices are connected to each other.

The switching then occurs on the “other” side.

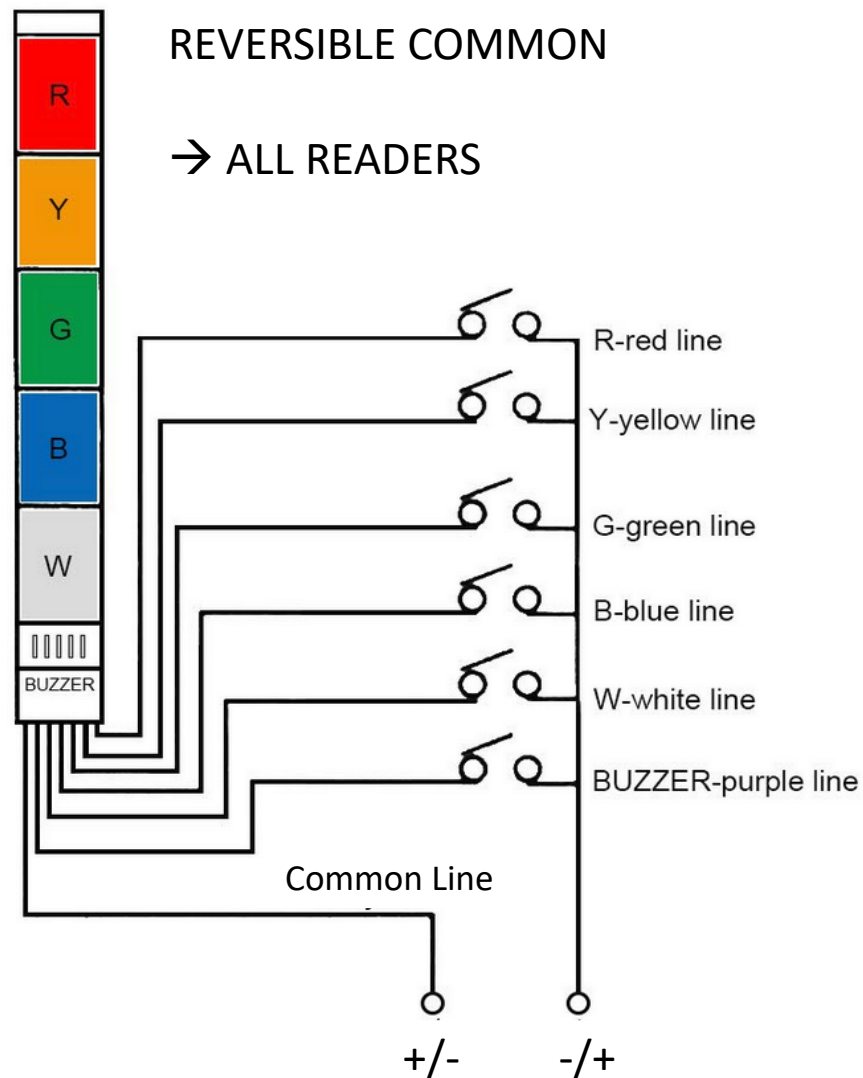


Figure 10 A REVERSIBLE COMMON configuration. This can work with all SensThys readers.

